

FIGURE 2 .

FIGURE 3

File No.: 1780/1G910-US3

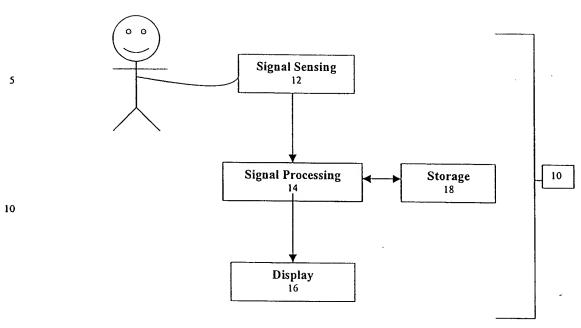
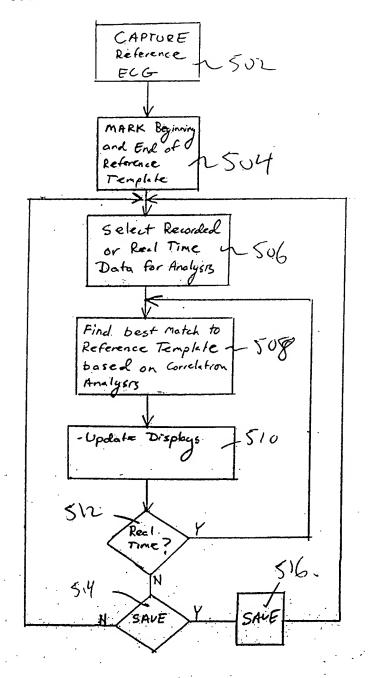


Figure 4

15

FIGURE 5 -




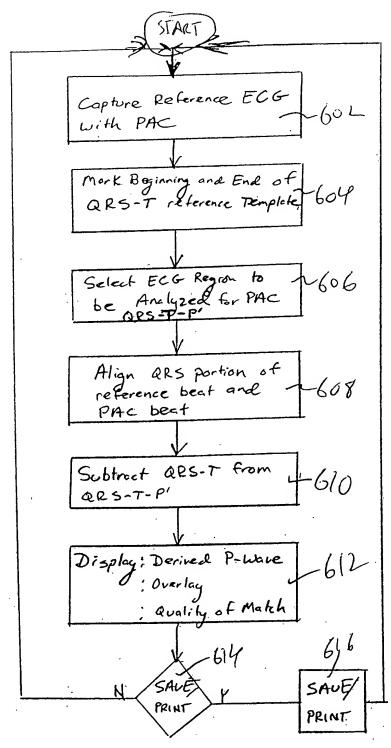



FIGURE 6


Figure 7

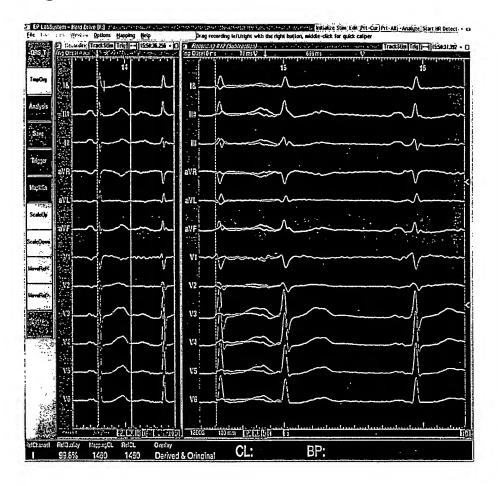

File No.: 1780/1G910-US3

## 5 Figure 8

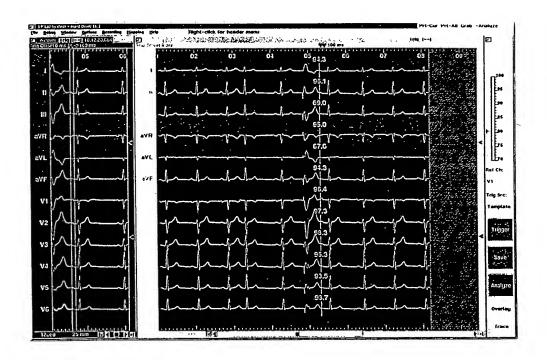

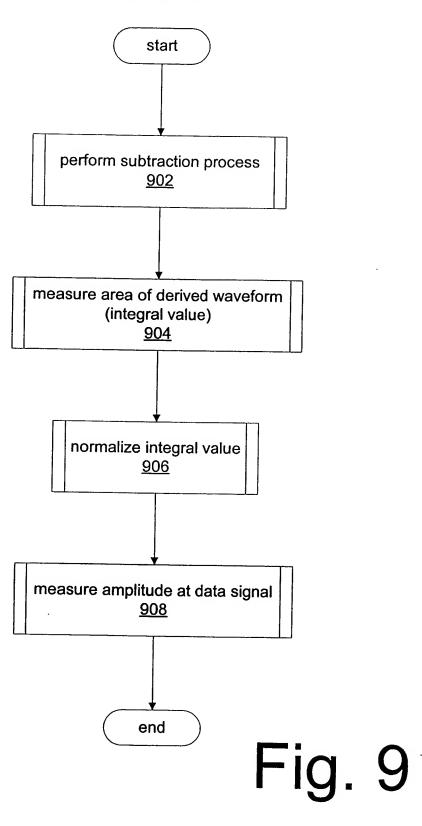

. F19. 8A

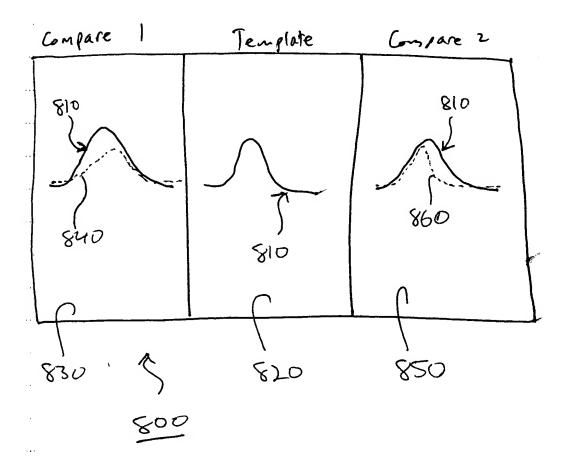


Fig. 10 (a)-(c) File No.: 1780/1G910-US3 (a) Trigger and Offset No continuous data stream P-ware Template P-wave template matching is processed along the entire incoming data stream Trigger and offset Defined by User Trigger defined as pea provave template defined as zoomsec. (c) Trigger and Offset Template Matching 1010 1030 1010


Inventor(s) David MacAdam

· FIGURE 11


64




ECG lead 1

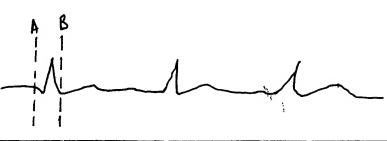


ECG lead 11




ECG lead III



Infracardiac lead 1



Intracadiac lead 2

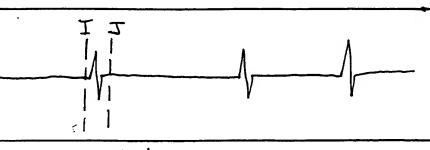

Intracaduce lead 3

